


# Shoelace Technique Guide


## Six Anchor Technique

**Step 1**

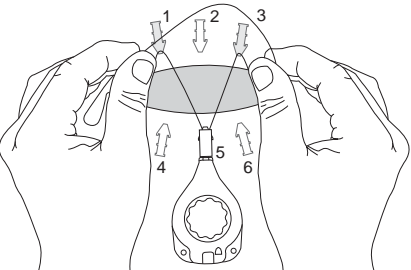


Seat tension controller under tab of home anchor (#5), loop line under anchor tab #1 and 3.

**Step 2**

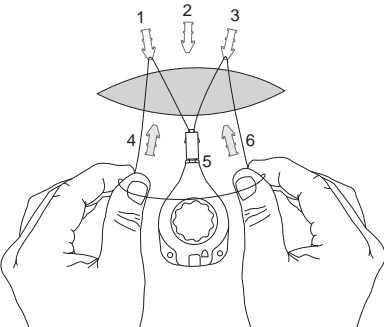

Loop line under anchor tab #4 and 6.


**Step 3**

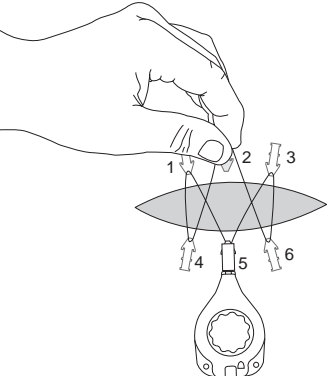

Loop remaining line under tab on anchor #2, turn blue control knob clockwise until audible clicking is heard (approx. 12 full rotations).


## Eight Anchor Technique

**Step 1**

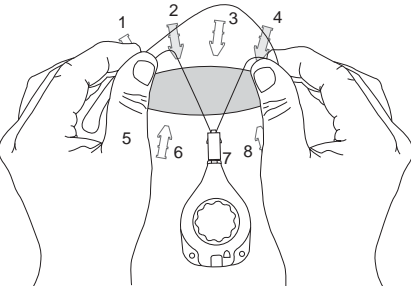


Seat tension controller under tab of anchor #7 (#6 could also be used), loop line under anchor tab #2 and 4.

**Step 2**

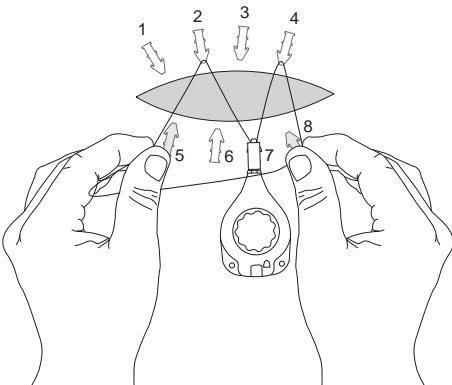


Loop line under anchor tab under #5 and 8.

**Step 3**

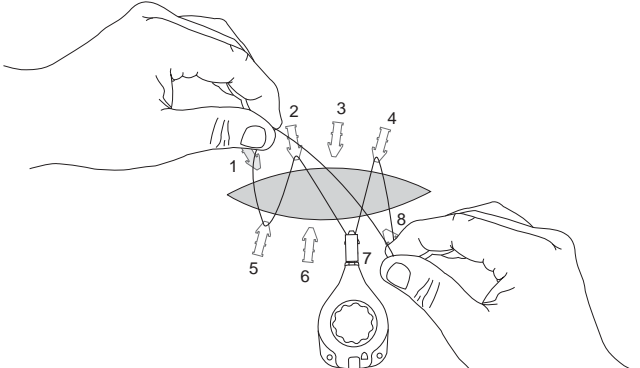


With left hand loop line under anchor tab #1 while pausing at anchor #8 with right hand.

**Step 4**

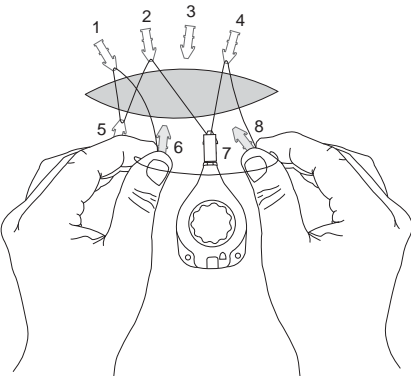


With left hand loop line under anchor tab #6 while #8 (right hand) remains paused.

**Step 5**

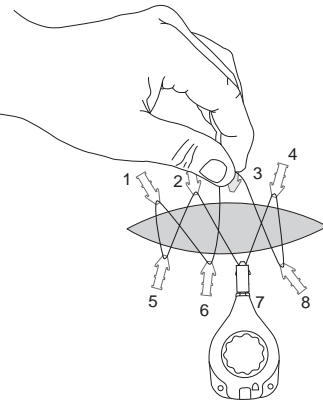

Loop remaining line under tab on anchor #3, turn blue control knob until audible clicking is heard (approx. 12 full rotations).

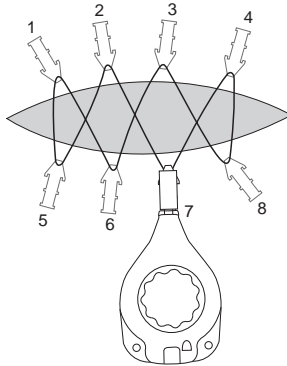


NOTE: For wounds longer than 10 cm and/or wider than 5 cm multiple devices may be used in series.  
DR-0084\_B

# Shoelace Technique Guide


## Ten Anchor Technique

**Step 1**

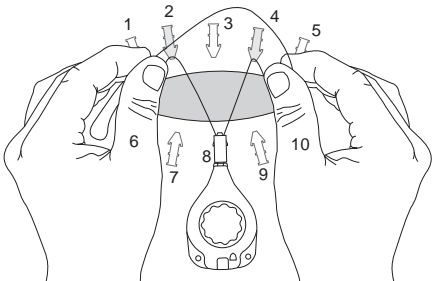


Seat tension controller under tab of home anchor (#8), loop line under anchor tab #2 and 4.

**Step 2**

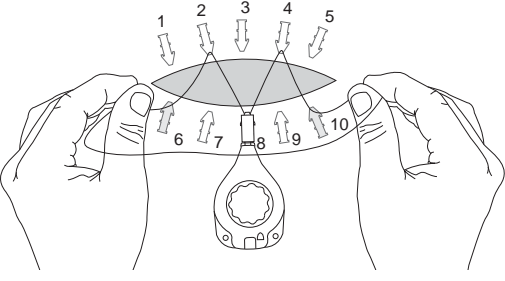


Loop line under anchor tab #6 and 10.

**Step 3**

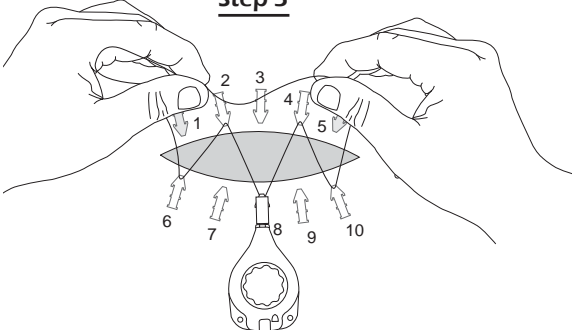


Loop line under anchor tab #1 and 5.

**Step 4**

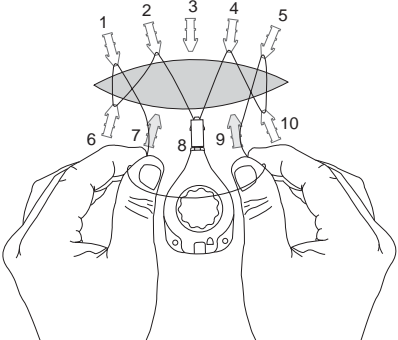


Loop line under anchor tab #7 and 9.

**Step 5**

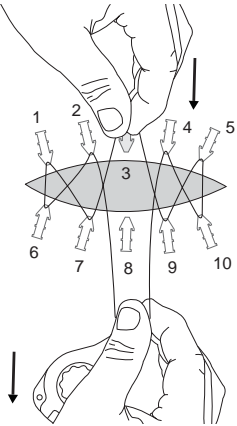

To take up slack pull tension controller while allowing line to loop under anchor tab #3.


**Step 6**

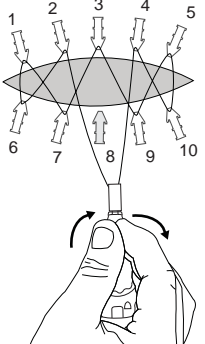

To take up remaining slack turn tension controller clockwise and seat into home anchor #8.


## End Position Technique

**Step 1**

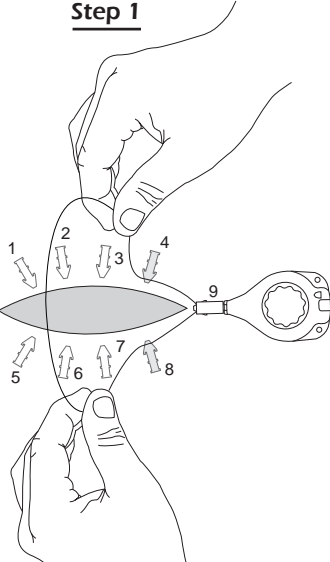


At one end of the wound seat tension controller under tab of anchor #9 loop tension line under tabs of first opposing anchors #4 and 8.

**Step 2**

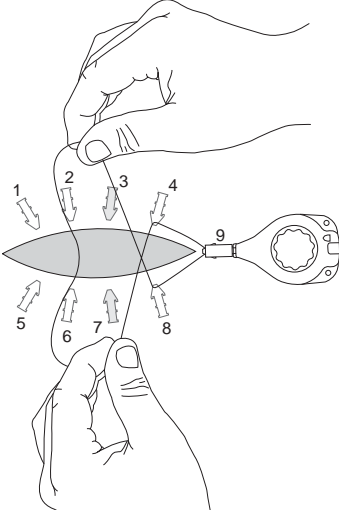


Cross line and loop on second set of opposing anchors #7 and 3.

**Step 3**

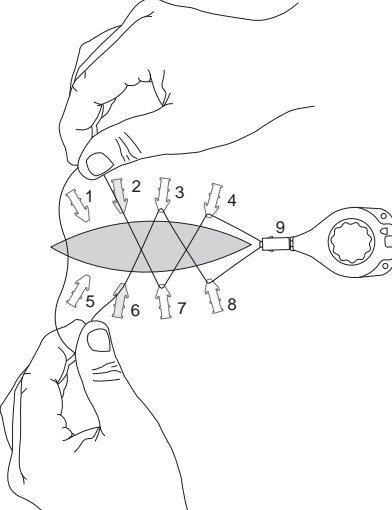


Cross line and loop on third set of opposing anchors #6 and 2.

**Step 4**

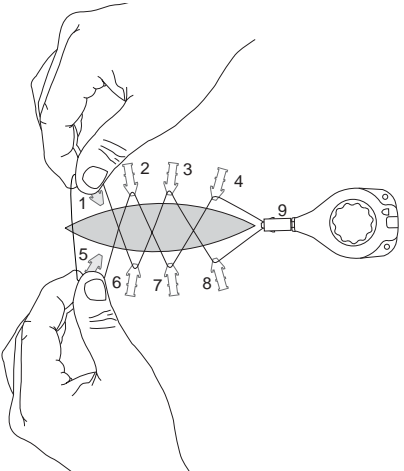

Cross line and loop on fourth set of opposing anchors #5 and 1 to take up remaining slack turn tension controller clockwise and seat into home anchor #9.

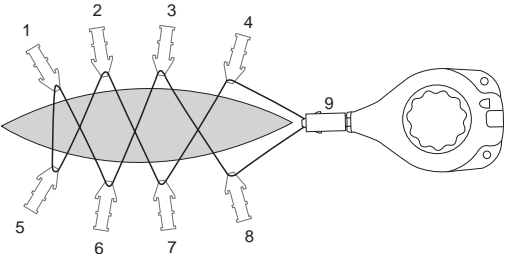

NOTE: For wounds longer than 10 cm and/or wider than 5 cm multiple devices may be used in series.